

Checklist for changes under MDR article 120.3

Background

Article 120(3) of (EU) 2017/745 (MDR) allows that devices in accordance with 93/42/EEC (MDD) can continue to be placed on the market if:

- The relevant MDD certificates are valid
- The devices continue to be compliant with MDD
- The following requirements of the MDR are met:
 - post-market surveillance (including PPRC),
 - vigilance,
 - registration of site and products, and
 - no significant changes to the design and the intended purpose.

This checklist is used to determine if the change in the intended purpose or design of the device is a significant as per article 120(3).

Requirements and responsibilities

This guidance is used for MDR article 120(3) and is to be completed in addition to the requirements in NBOG BPG 2014-3 “Guidance for manufacturers and Notified Bodies on reporting design changes and changes of quality system”.

When using this checklist, the following mandatory instructions apply:

- Any change made to the approved design or intended purpose of an existing MDD product under article 120(3) of MDR must be assessed within this checklist.
- This checklist is to be approved by the person responsible for regulatory compliance (PRRC).
- The checklist consists of 6 flowcharts (taken from MDCG 2020-3):
 - Main Chart
 - Flow Chart A: Intended purpose
 - Flow Chart B: Design and performance specification
 - Flow Chart C: Software
 - Flow Chart D: Material
 - Flow Chart E: Sterilization method or packaging design
- All charts must be completed for each change. If a chart is not applicable, it is to be justified in the footer of the chart.
- If a change includes multiple changes, each change must be assessed on its own. In addition, the cumulative impact of changes must be assessed.
- Examples of significant and non-significant changes and further guidance are given in MDCG Guidance 2020-3.



Checklist for changes under MDR article 120.3

- If the assessment concludes that the change is significant, the change process shall be discontinued. Decision must be made by top management if and how to follow-up the change.
- The notified body will have to be notified of any change for class III or active implantable devices.
 - Using this checklist, we will determine if the change is significant or not.
 - Non-significant changes will be notified to our notified body. The notified body will review and agree or disagree to our notification.
 - The change can only be implemented once the notified body agreed that the change is non-significant.
 - The non-significant change will be listed continuously in the list of changes.
- All non-significant changes for class I and class II devices will be listed continuously in the list of changes
 - The list of non-significant changes to class I and class II products will be submitted, if requested, to the notified body ahead of the annual surveillance audits.

References


[1] (EU) 2017/745 MDR

[2] NBOG BPG 2014-3 “Guidance for manufacturers and Notified Bodies on reporting design changes and changes of quality system”

[3] MDCG 2020-3 Guidance on significant changes regarding the transitional provision under Article 120 of the MDR with regard to devices covered by certificates according to MDD or AIMDD

Checklist for changes under MDR article 120.3


Main chart (Part 1)

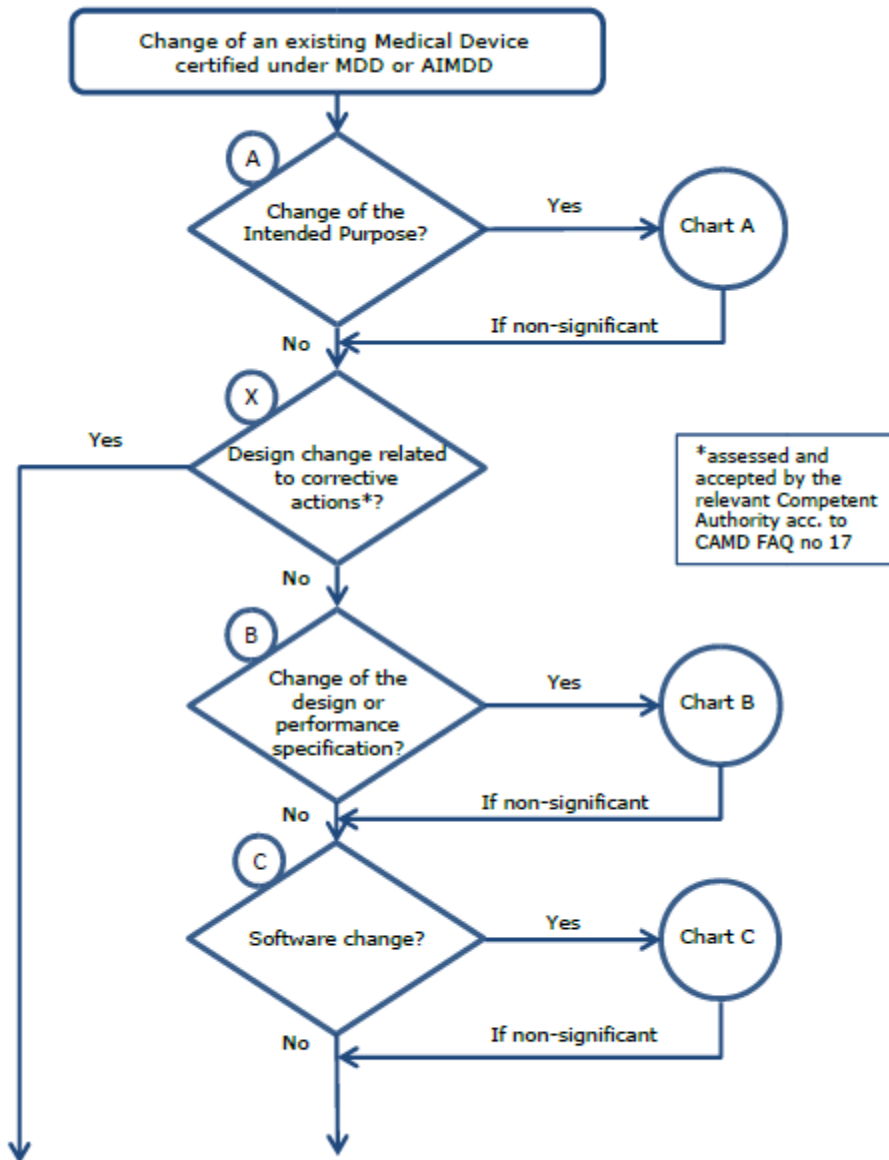

Main chart (Part 2)

Checklist for changes under MDR article 120.3

Main chart (Part 2)

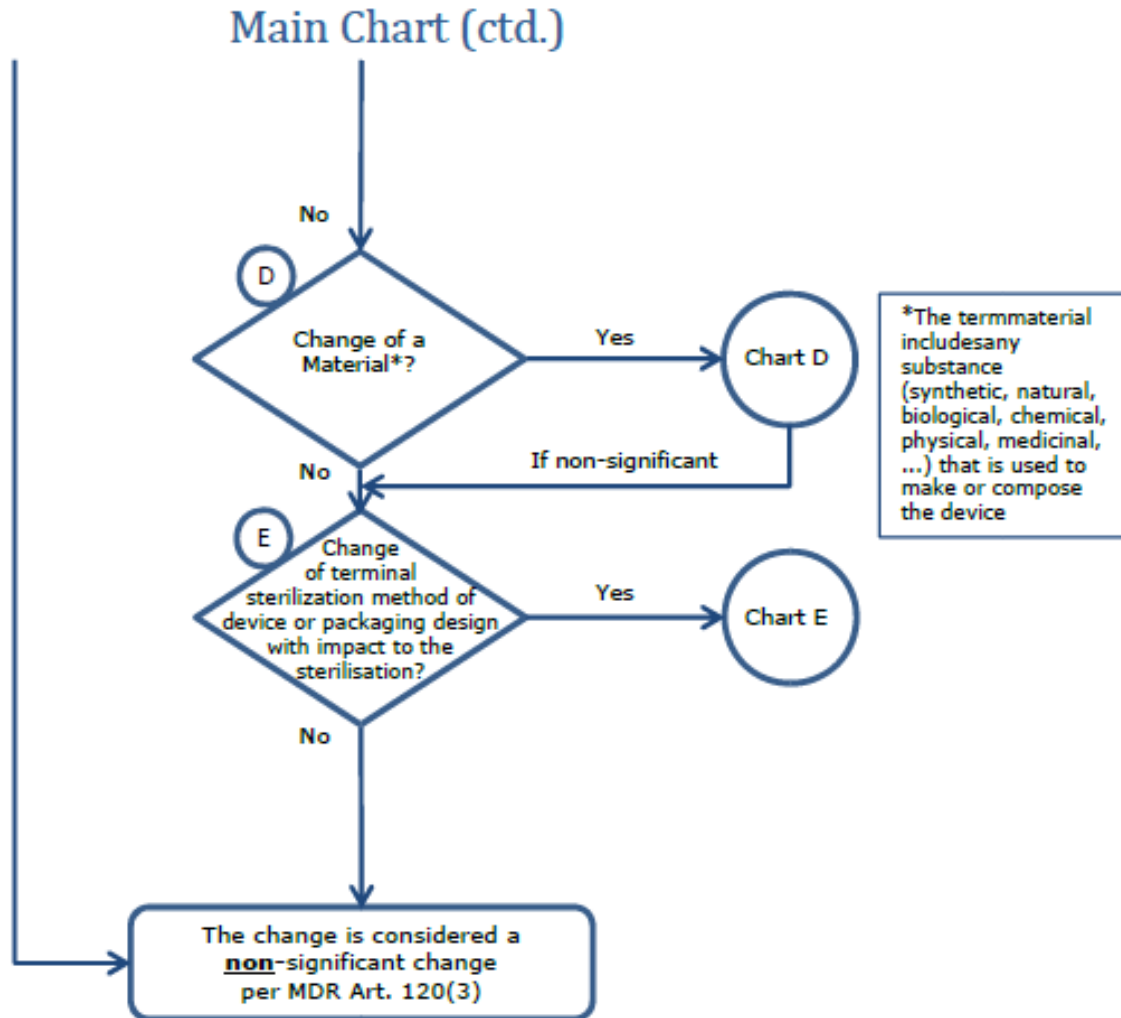


Conclusion:

The change is significant yes no

Checklist for changes under MDR article 120.3

Flow Chart A: Intended purpose

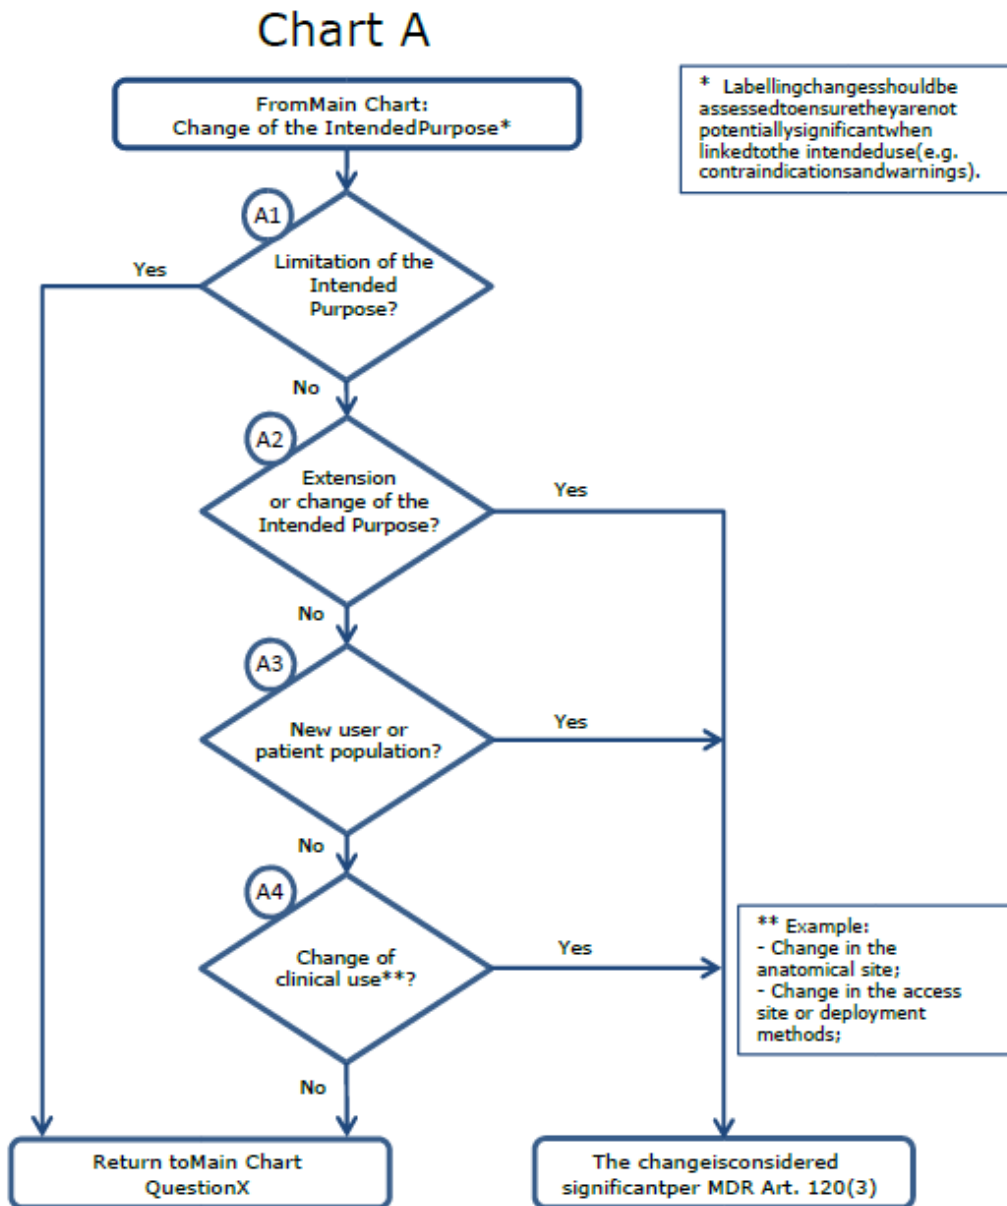


Conclusion:

The flowchart is not applicable because:

The change is significant yes no

Checklist for changes under MDR article 120.3

Flow Chart B: Design and performance specification

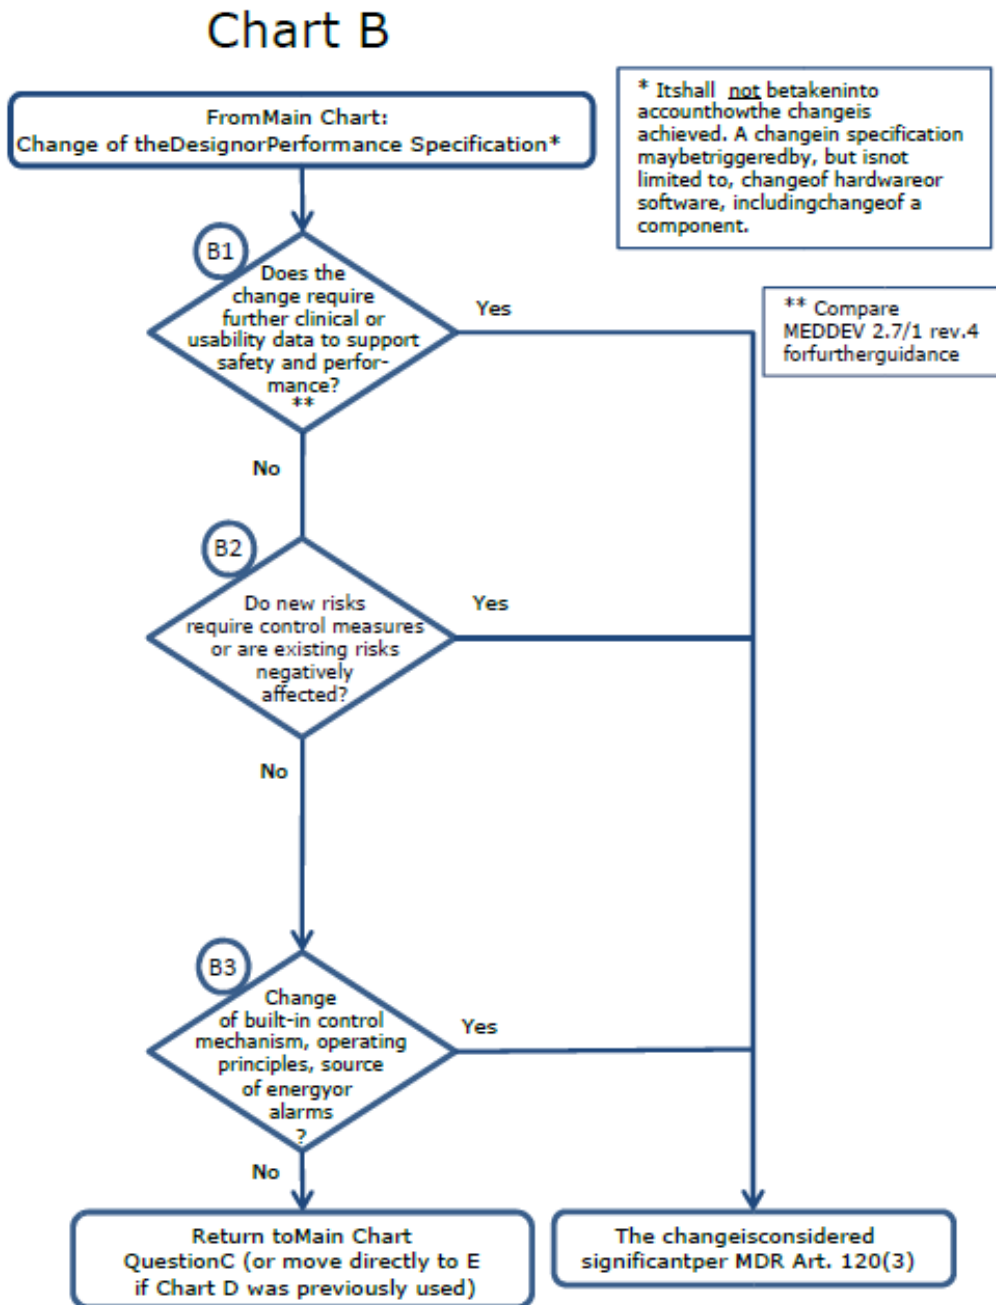

Conclusion:


The flowchart is not applicable because:

The change is significant yes no

Checklist for changes under MDR article 120.3

Flow Chart C: Software (Part 1)

Chart C

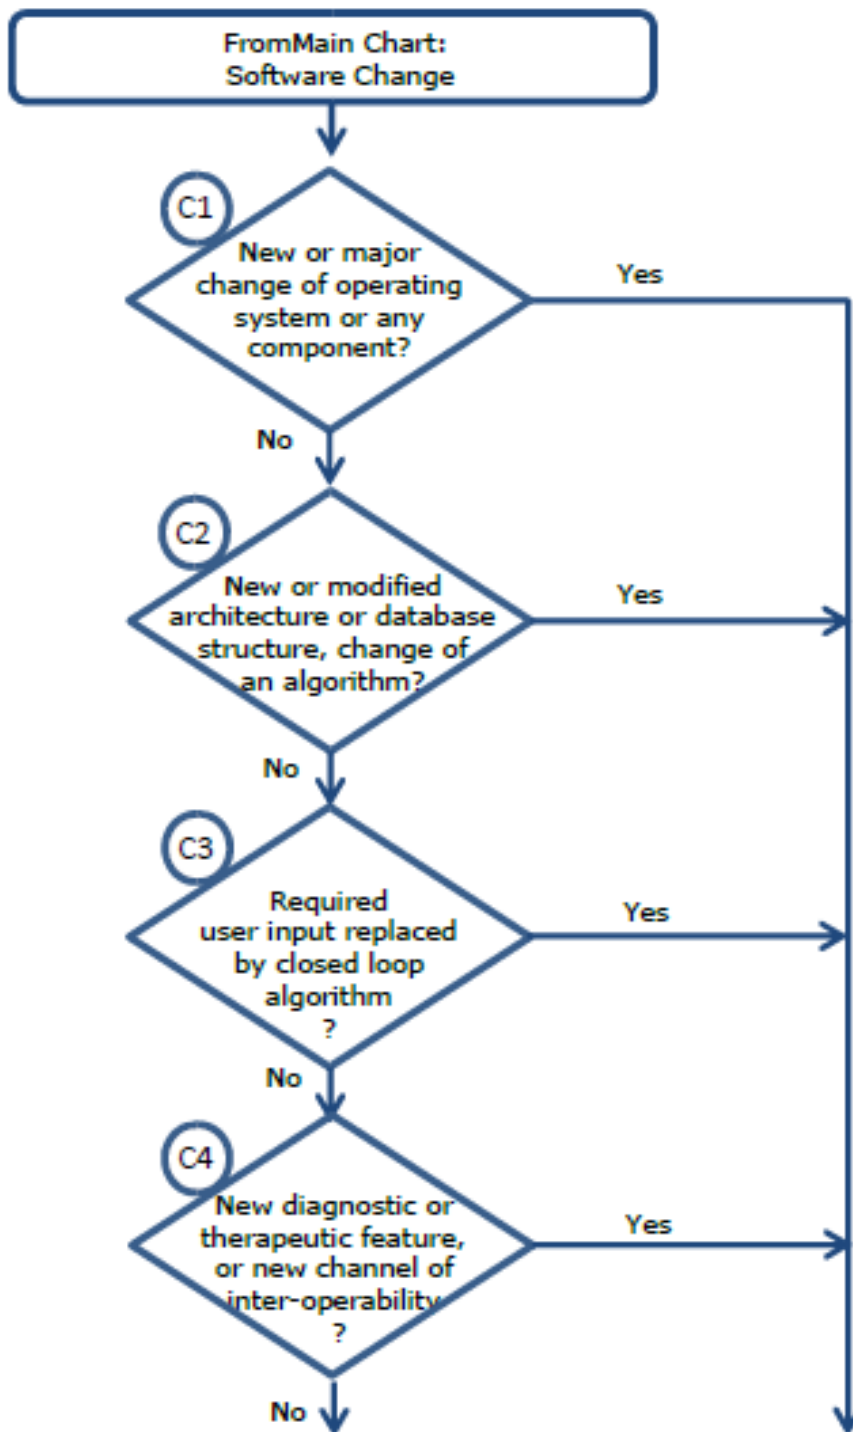


Software (Part 2)

Checklist for changes under MDR article 120.3

Flow Chart C: Software (Part 2)

Chart C (ctd.)

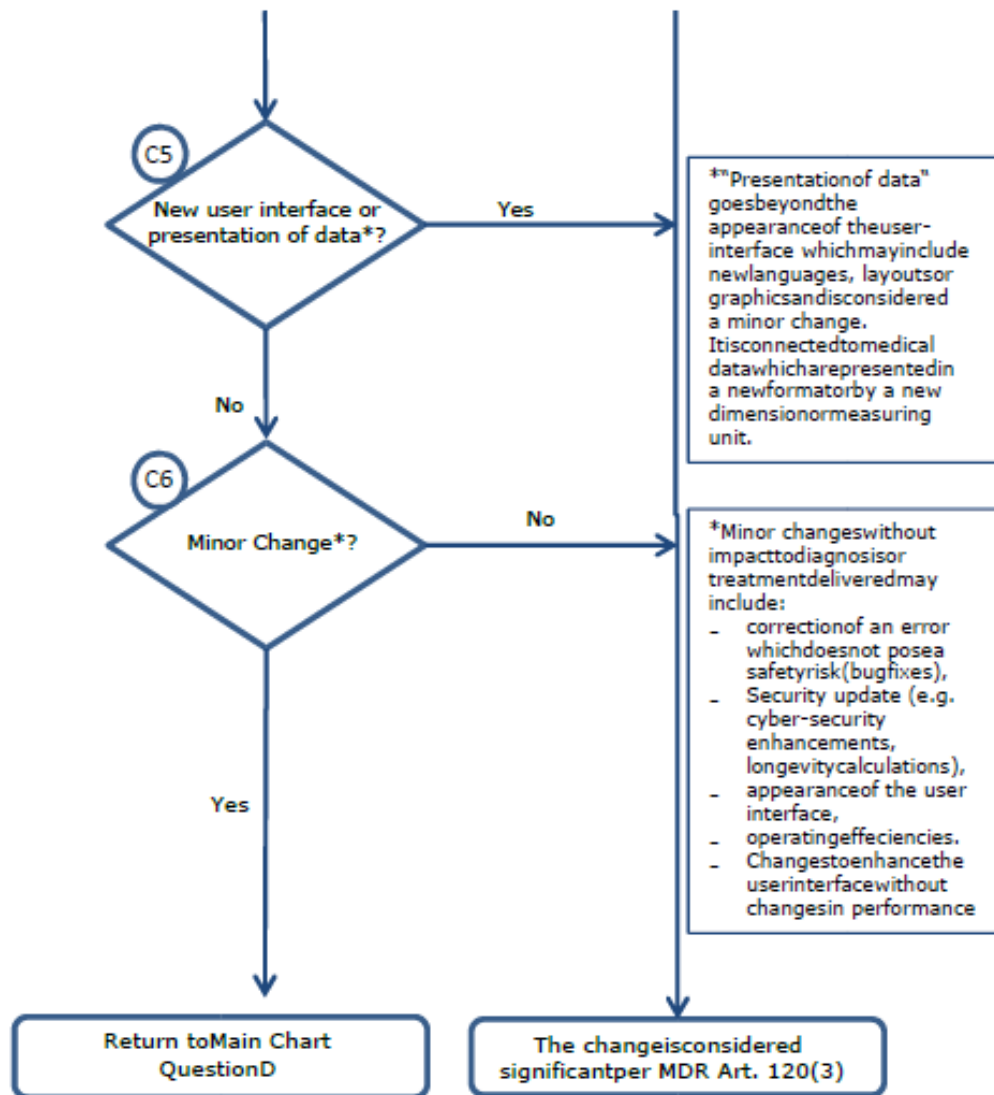


Conclusion:

The flowchart is not applicable because:

The change is significant yes no

Checklist for changes under MDR article 120.3


Flow Chart D: Material (Part 1)

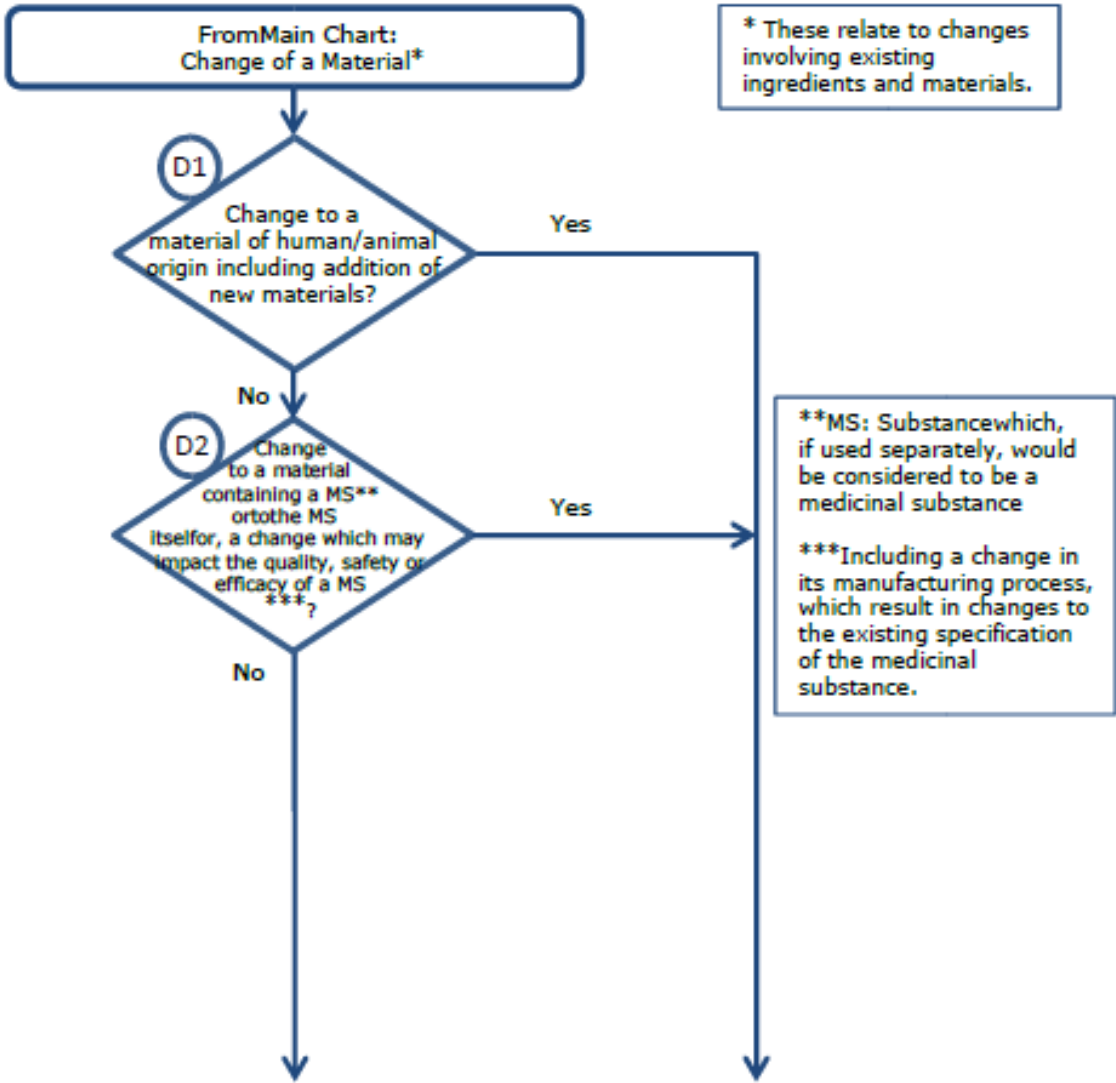

Material (Part 2)

Checklist for changes under MDR article 120.3

Flow Chart D: Material (Part 2)

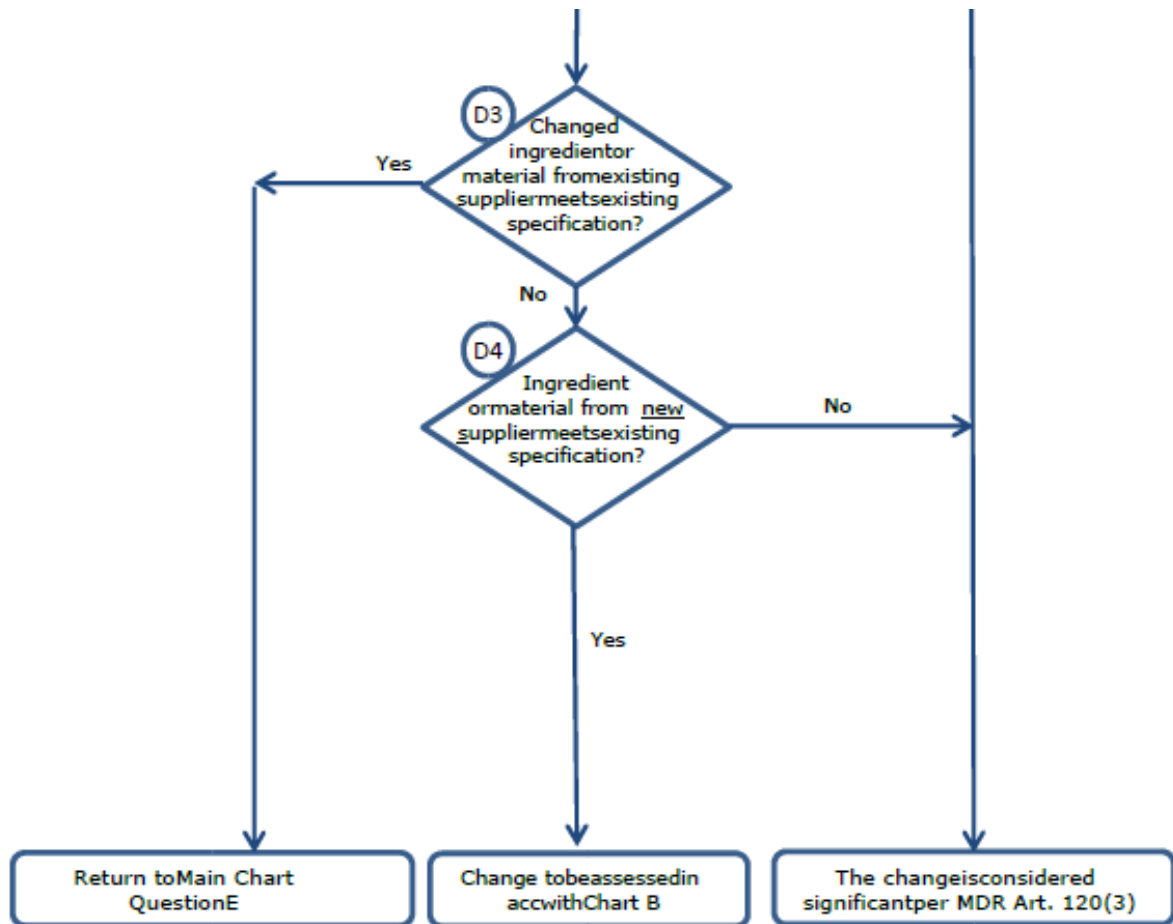


Conclusion:

The flowchart is not applicable because:

The change is significant yes no

Checklist for changes under MDR article 120.3

Flow Chart E: Sterilization method or packaging design

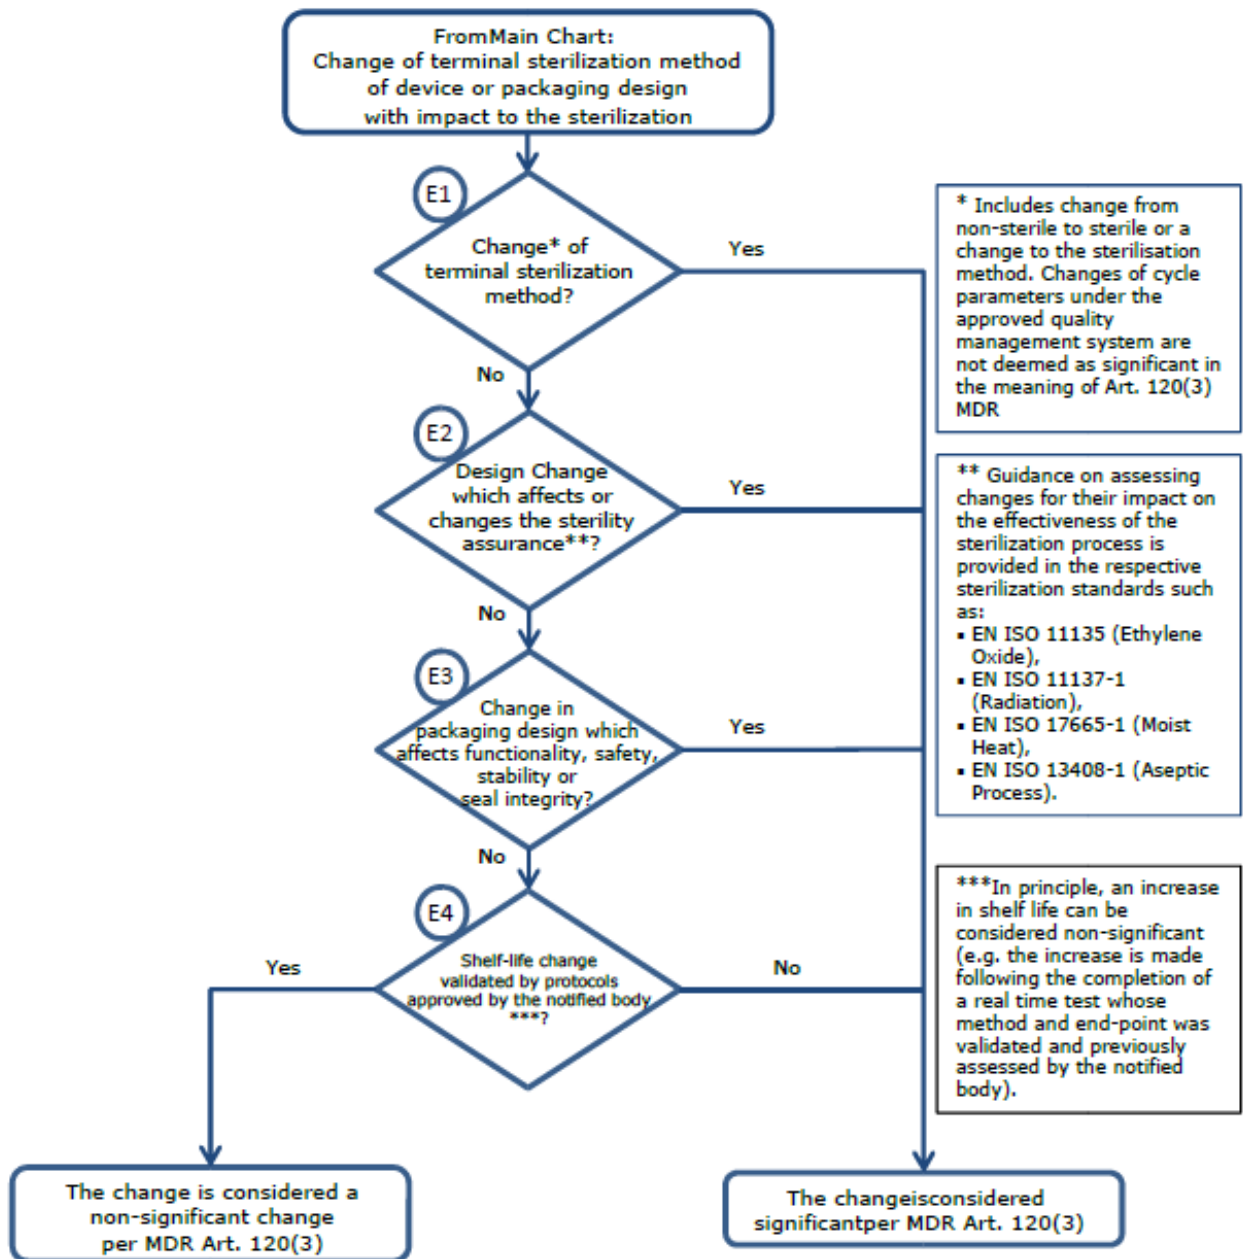

Conclusion:

The flowchart is not applicable because:

The change is significant yes no

Checklist for changes under MDR article 120.3

Conclusion:

The change is considered significant

yes no

In case of multiple changes within one assessment:

The cumulative impact of change is considered significant

yes no, because (justify):

The product is a class III product and/or active implantable device. Notification to notified body will have to be notified prior to implementation.

Change Notification number: _____

The product is a class I or class II device and notification to notified body is not needed prior to implementation.

Approval by PRRC

Date / Name / Signature